


USER'S MANUAL

BM805s
BM806s
BM807s

Practical Multimeters



BRYMEN
BRIGHT PEOPLE'S CHOICE

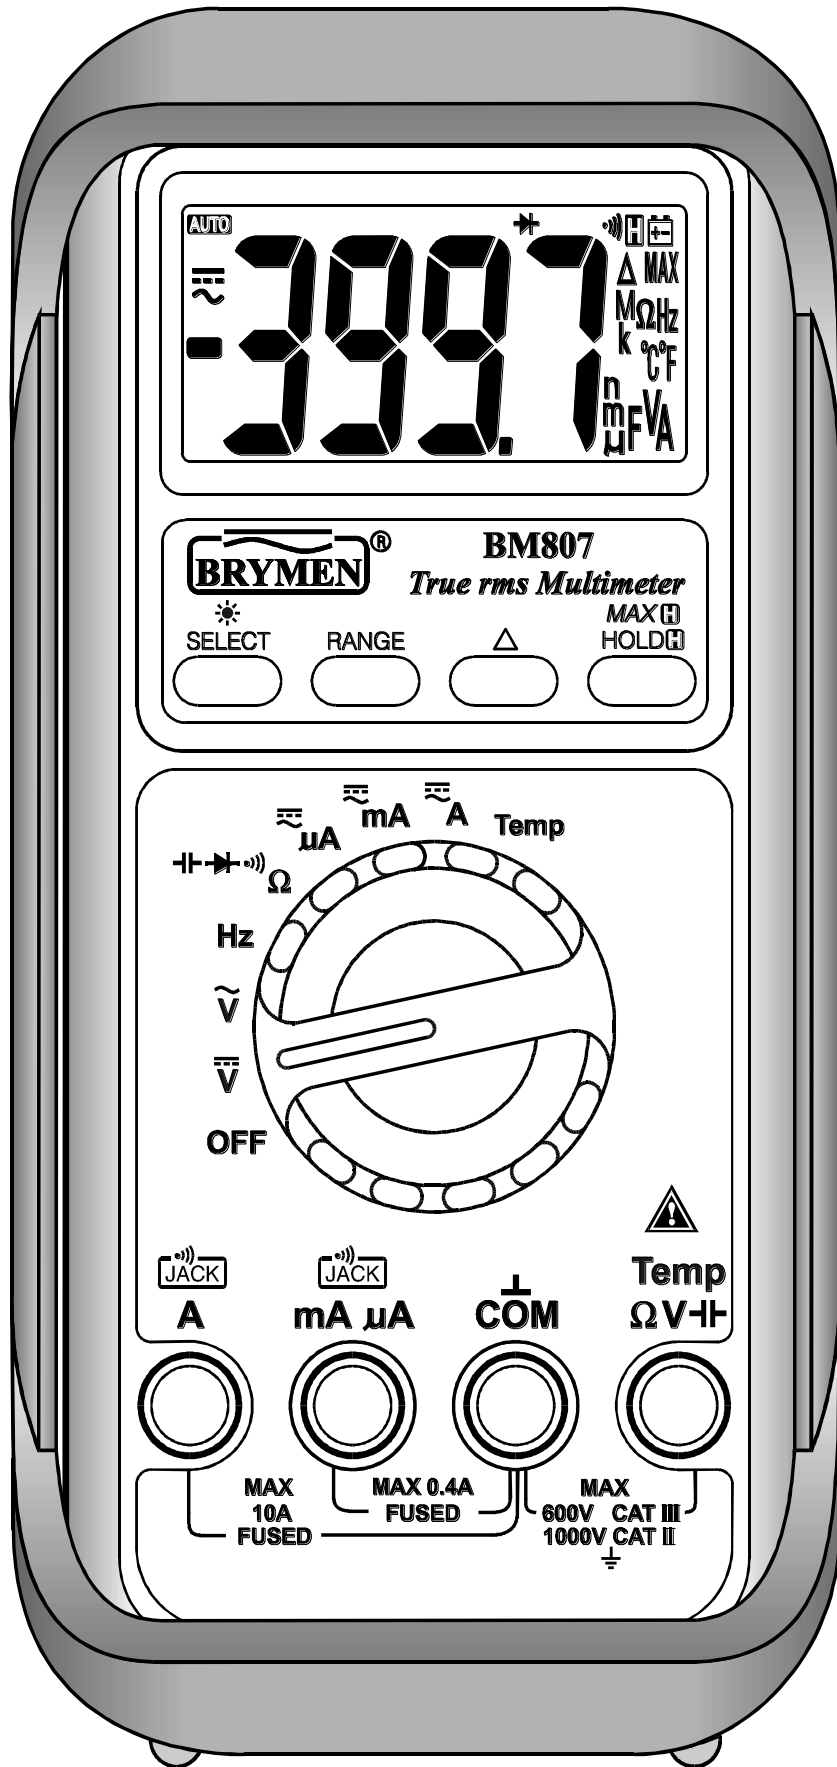

1) SAFETY

This manual contains information and warnings that must be followed for operating the instrument safely and maintaining the instrument in a safe operating condition. If the instrument is used in a manner not specified by the manufacturer, the protection provided by the instrument may be impaired. The meter is intended only for indoor use.

The meter protection rating, against the users, is double insulation per IEC/UL/EN61010-1 Ed. 3.0, IEC/EN61010-2-030 Ed. 1.0, IEC/EN61010-2-033 Ed. 1.0, IEC/UL/EN61010-031 Ed. 1.1 and CAN/CSA-C22.2 No. 61010-1-12 Ed. 3.0 to Category II 1000 Volts, CAT III 600Volts and CAT IV 300Volts AC & DC.

Terminals (to COM) measurement category:

V / A / mA μ A: Category II 1000V, Category III 600V and Category IV 300V AC & DC.

Per IEC61010-1 2nd Ed. (2001) Measurement Category

Measurement Category IV (CAT IV) is for measurements performed at the source of the low-voltage installation. Examples are electricity meters and measurements on primary overcurrent protection devices and ripple control units.

Measurement Category III (CAT III) is for measurements performed in the building installation. Examples are measurements on distribution boards, circuit-breakers, wiring, including cables, bus-bars, junction boxes, switches, socket-outlets in the fixed installation, and equipment for industrial use and some other equipment, for example, stationary motors with permanent connection to the fixed installation.

Measurement Category II (CAT II) is for measurements performed on circuits directly connected to the low voltage installation. Examples are measurements on household appliances, portable tools and similar equipment.

Terms in this manual:

WARNING identifies conditions and actions that could result in serious injury or even death to the user.

CAUTION identifies conditions and actions that could cause damage or malfunction in the instrument.








WARNING

To reduce the risk of fire or electric shock, do not expose this product to rain or moisture. To avoid electrical shock hazard, observe the proper safety precautions when working with voltages above 60 VDC or 30 VAC rms. These voltage levels pose a potential shock hazard to the user. Do not touch test lead tips or the circuit being tested while power is applied to the circuit being measured. Keep your fingers behind the finger guards of the test leads during measurement. Inspect test leads, connectors, and probes for damaged insulation or exposed metal before using the instrument. If any defects are found, replace them immediately. Do not measure any current that exceeds the current rating of the protection fuse(s). Do not attempt a current measurement to any circuit where the open circuit voltage is above the protection fuse(s) voltage rating(s). Suspected open circuit voltage should be checked with voltage functions. Never attempt a voltage measurement with the test lead inserted into the $\mu\text{A}/\text{mA}$ or A input jack. Only replace the blown fuse(s) with the proper rating as specified in this manual. **Only use the test lead provided with the equipment or UL Listed Probe Assembly.**

CAUTION

Disconnect the test leads from the test points before changing functions. Always set the instrument to the highest range and work downward for an unknown value when using manual ranging mode.

INTERNATIONAL ELECTRICAL SYMBOLS


	Caution ! Refer to the explanation in this Manual
	Caution ! Risk of electric shock
	Earth (Ground)
	Double Insulation or Reinforced insulation
	Fuse
	AC--Alternating Current
	DC--Direct Current

2) CENELEC DIRECTIVES

The instruments conform to CENELEC Low-voltage directive **2006/95/EC** and Electromagnetic compatibility directive **2004/108/EC**


3) PRODUCT DESCRIPTION

This user's manual uses only representative model for illustrations. Please refer specification details for function availability to each model.

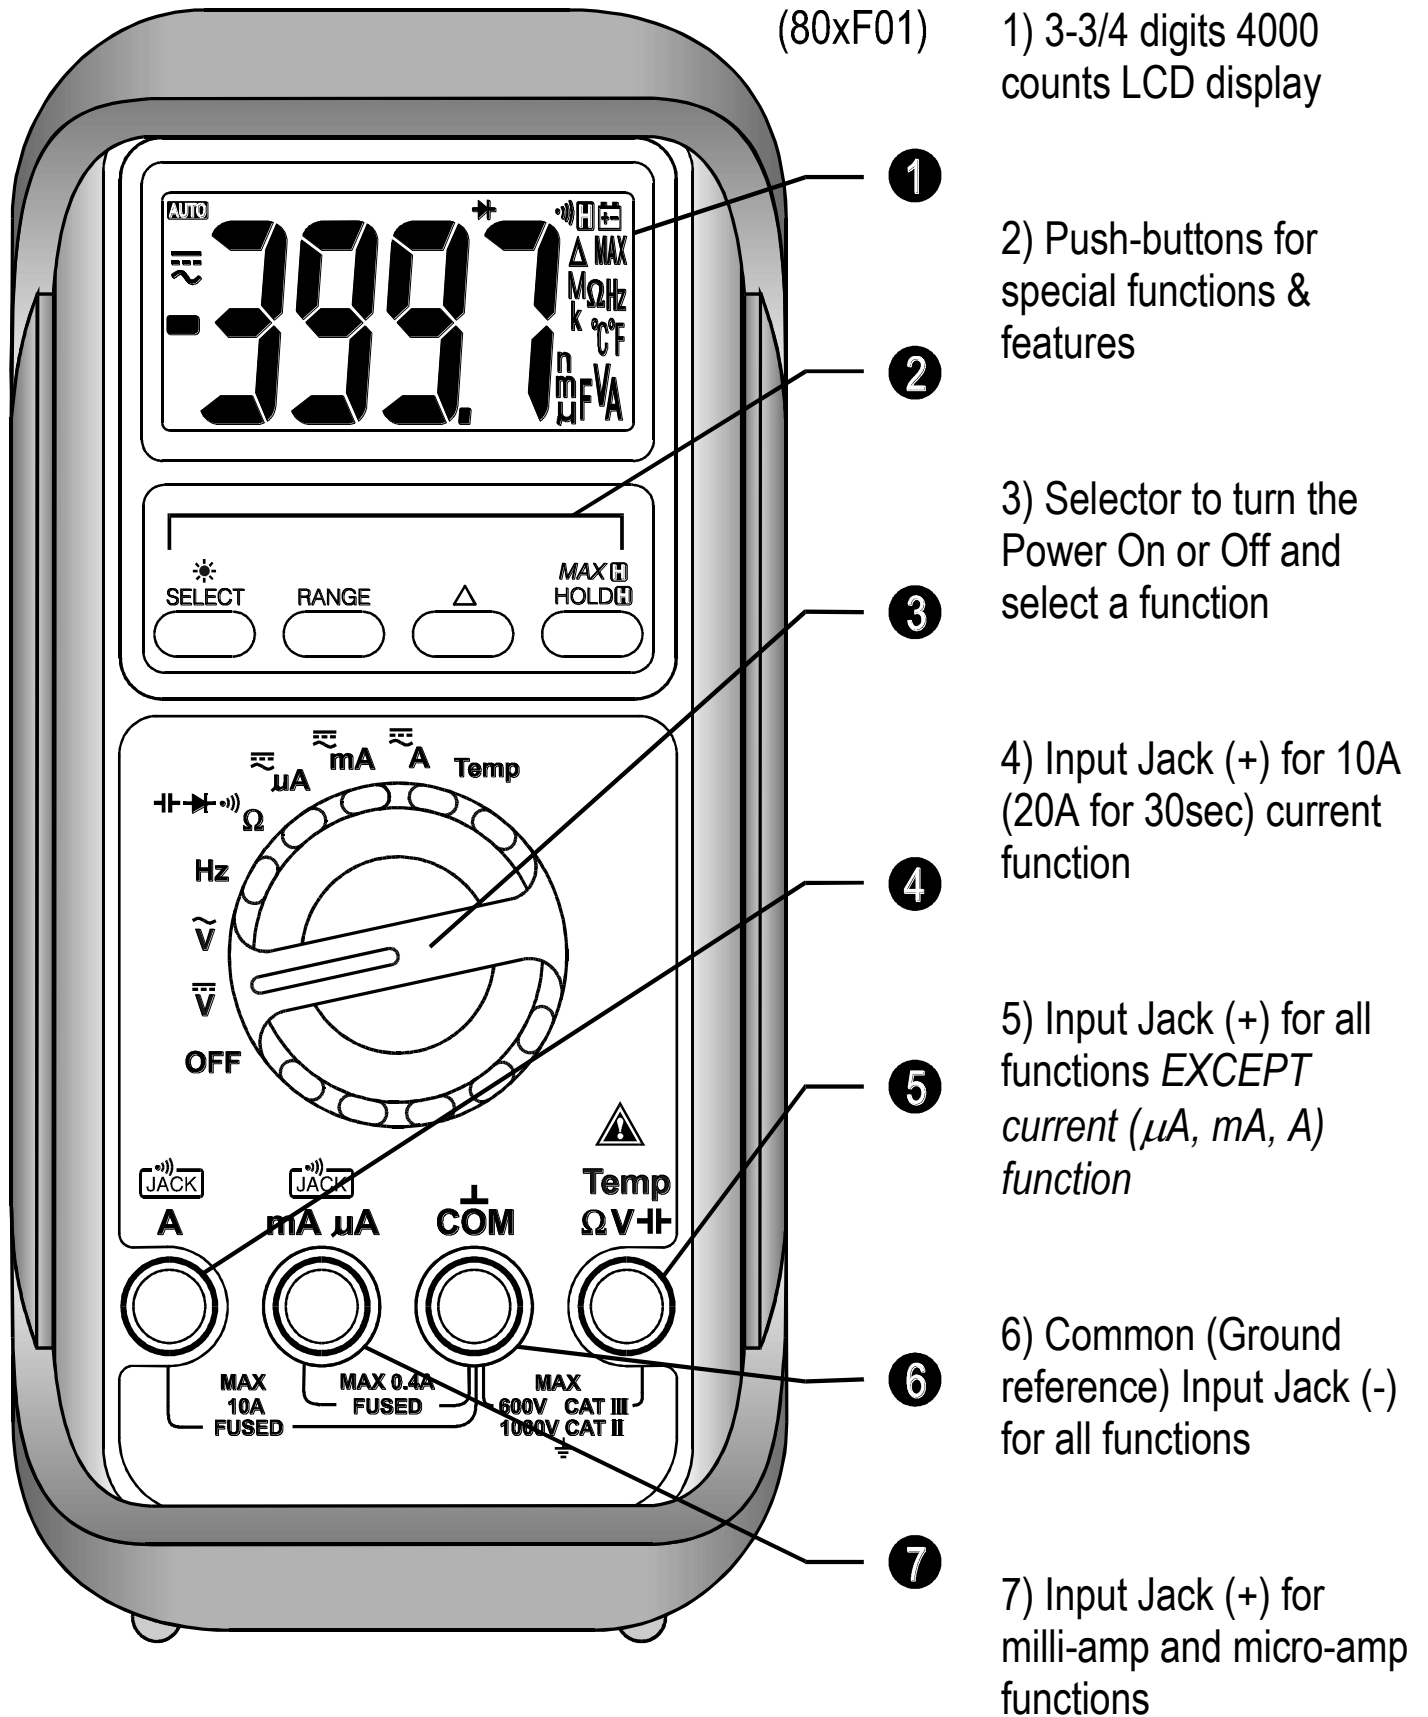

4) OPERATION

DC Voltage, AC Voltage, & Hz Frequency functions

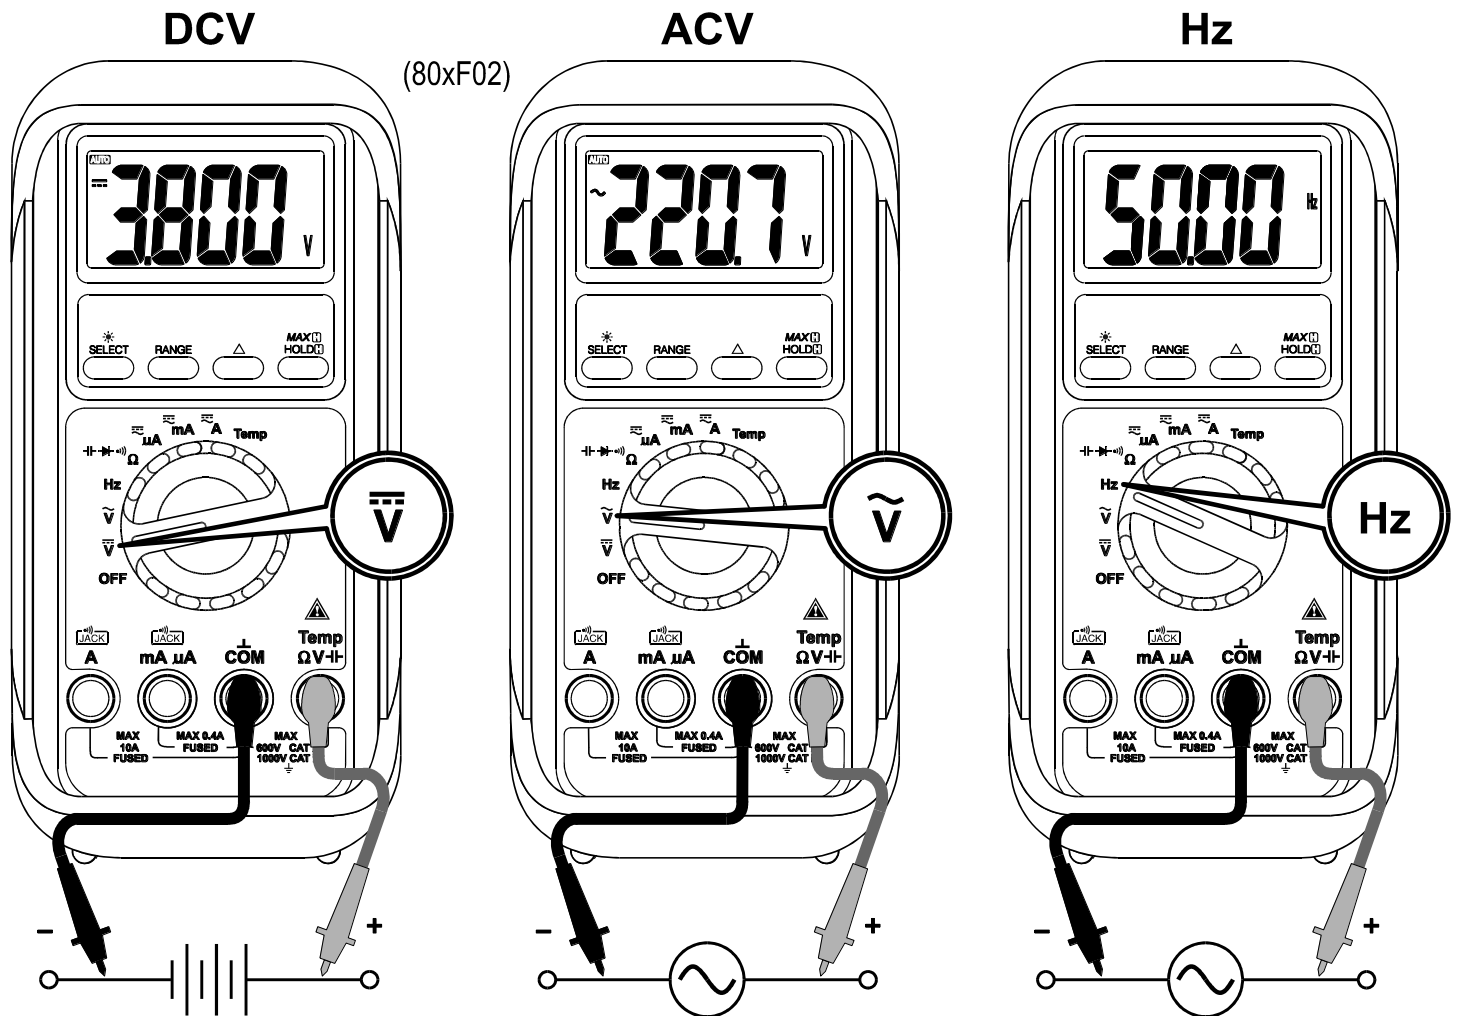

CAUTION

Before and after hazardous voltage measurements, test the voltage function on a known source such as line voltage to determine proper meter functioning.


Note:

1) AC 400.0mV range selection is by RANGE button manually, and is specified from AC 10mV (AC 40mV for True RMS model **Model 807s**) and up.

2) DC 400.0mV range is designed with 1000MΩ high input impedance for least current drain in measuring small signals, and can cope better with most commercially available voltage output transducers and adapters. The non-zero display reading is normal when the meter inputs are open circuit, which will not affect actual measurement accuracy. Open input is actually a floating condition, which is not a zero-volt-input condition. The meter will show zero or close to zero reading when the inputs are shorted.

Ω Resistance, and $\cdot\cdot\cdot$) Continuity functions

Defaults at Ω . Press **SELECT** button momentarily to select $\cdot\cdot\cdot$) Continuity function which is convenient for checking wiring connections and operation of switches. A continuous beep tone indicates a complete wire.

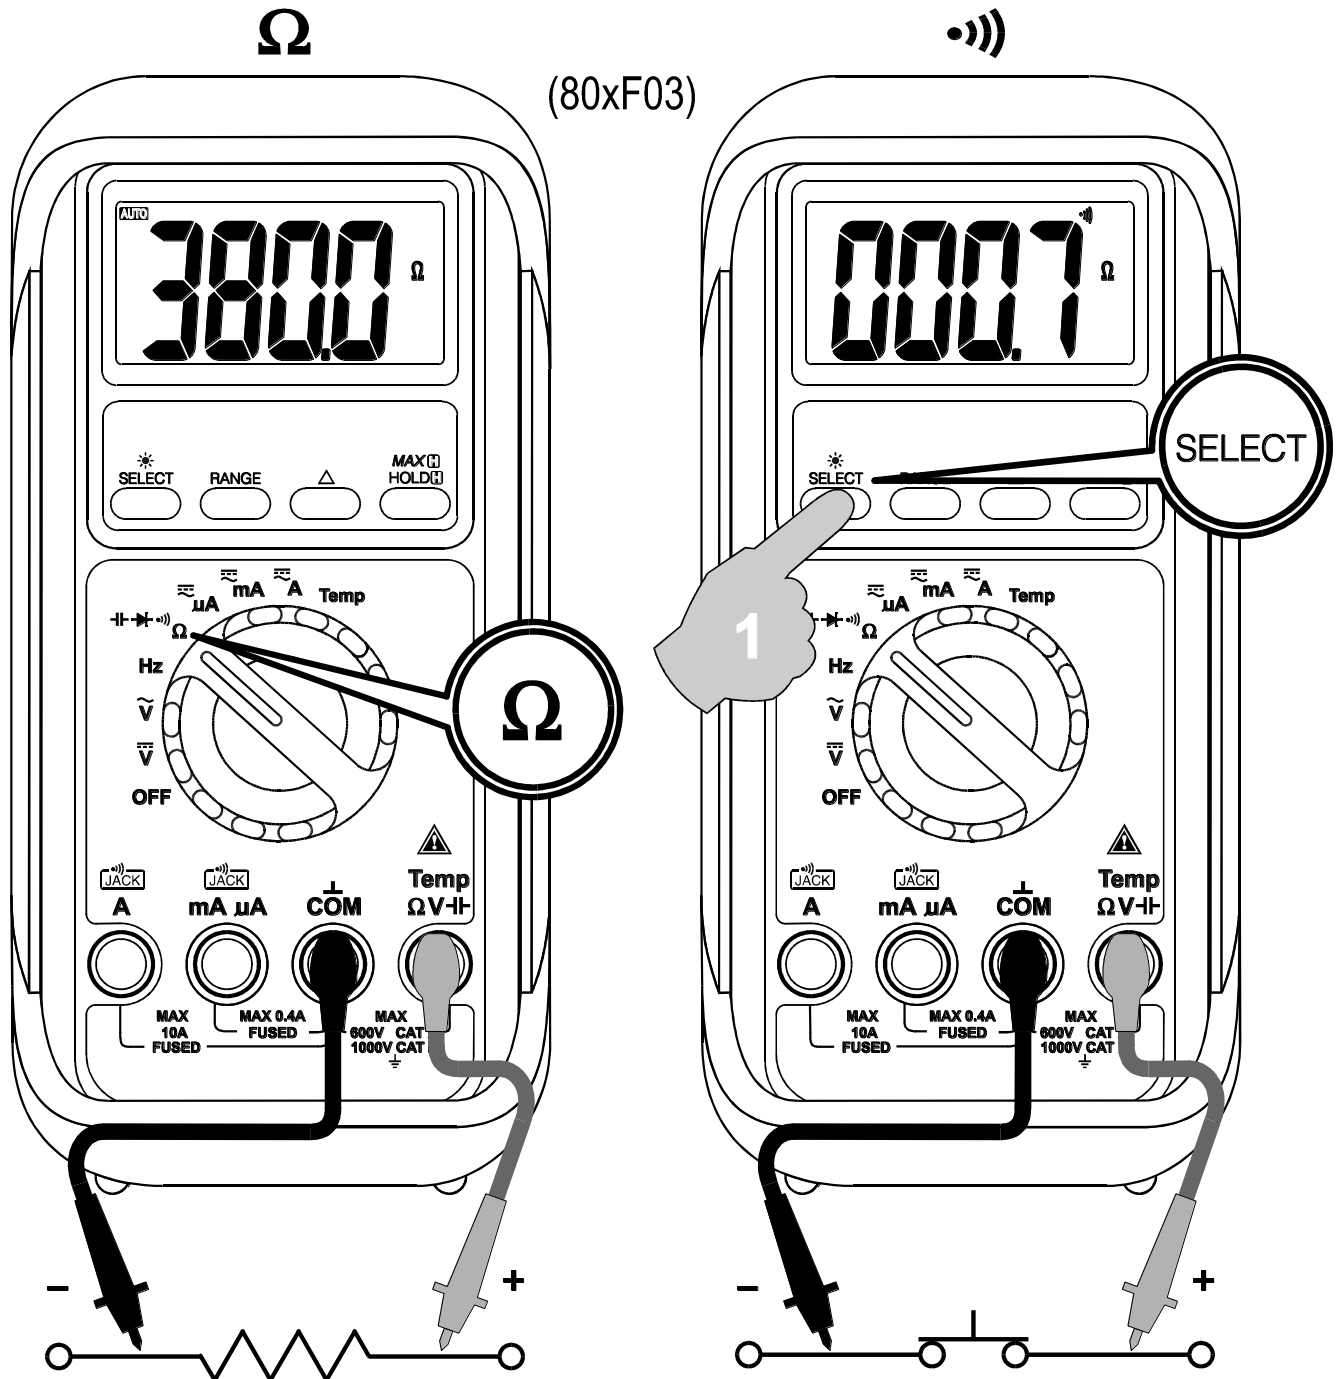


CAUTION

Using Resistance, Continuity, Diode or Capacitance function in a live circuit will produce false results and may damage the instrument. In many cases the suspected component must be disconnected from the circuit to obtain an accurate measurement reading.

➔ Diode test, ⇌ Capacitance functions

Defaults at Ω . Press **SELECT** button momentarily 2 times to select ➔ Diode test function. Normal forward voltage drop (forward biased) for a good silicon diode is between 0.400V to 0.900V. A reading higher than that indicates a leaky diode (defective). A zero reading indicates a shorted diode (defective). An OL indicates an open diode (defective). Reverse the test leads connections (reverse biased) across the diode. The digital display shows OL if the diode is good. Any other readings indicate the diode is resistive or shorted (defective).

Defaults at Ω . Press **SELECT** button momentarily 3 times to select ⇌ Capacitance function. Relative zero Δ mode can be used to zero out the parasitic capacitance of the leads and the internal protection circuitry of the meter when measuring low capacitance in the order of Pico Farad (pF).

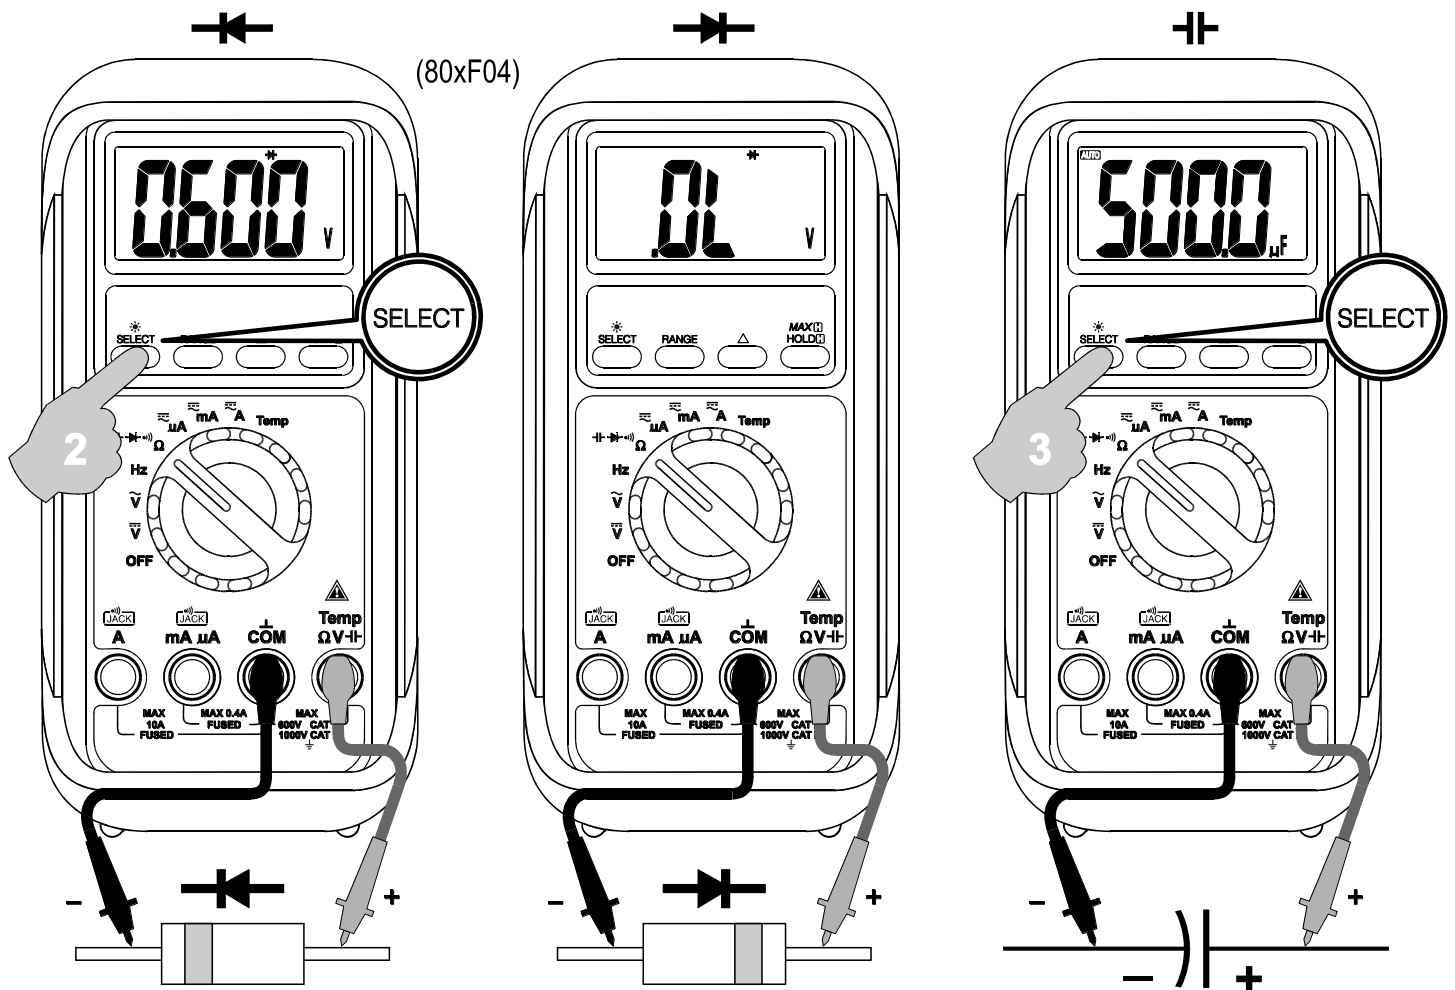


CAUTION

Discharge capacitors before making any measurement. Large value capacitors should be discharged through an appropriate resistance load

μA , mA, and A Current functions

Default at DC. Press **SELECT** button momentarily to select AC.

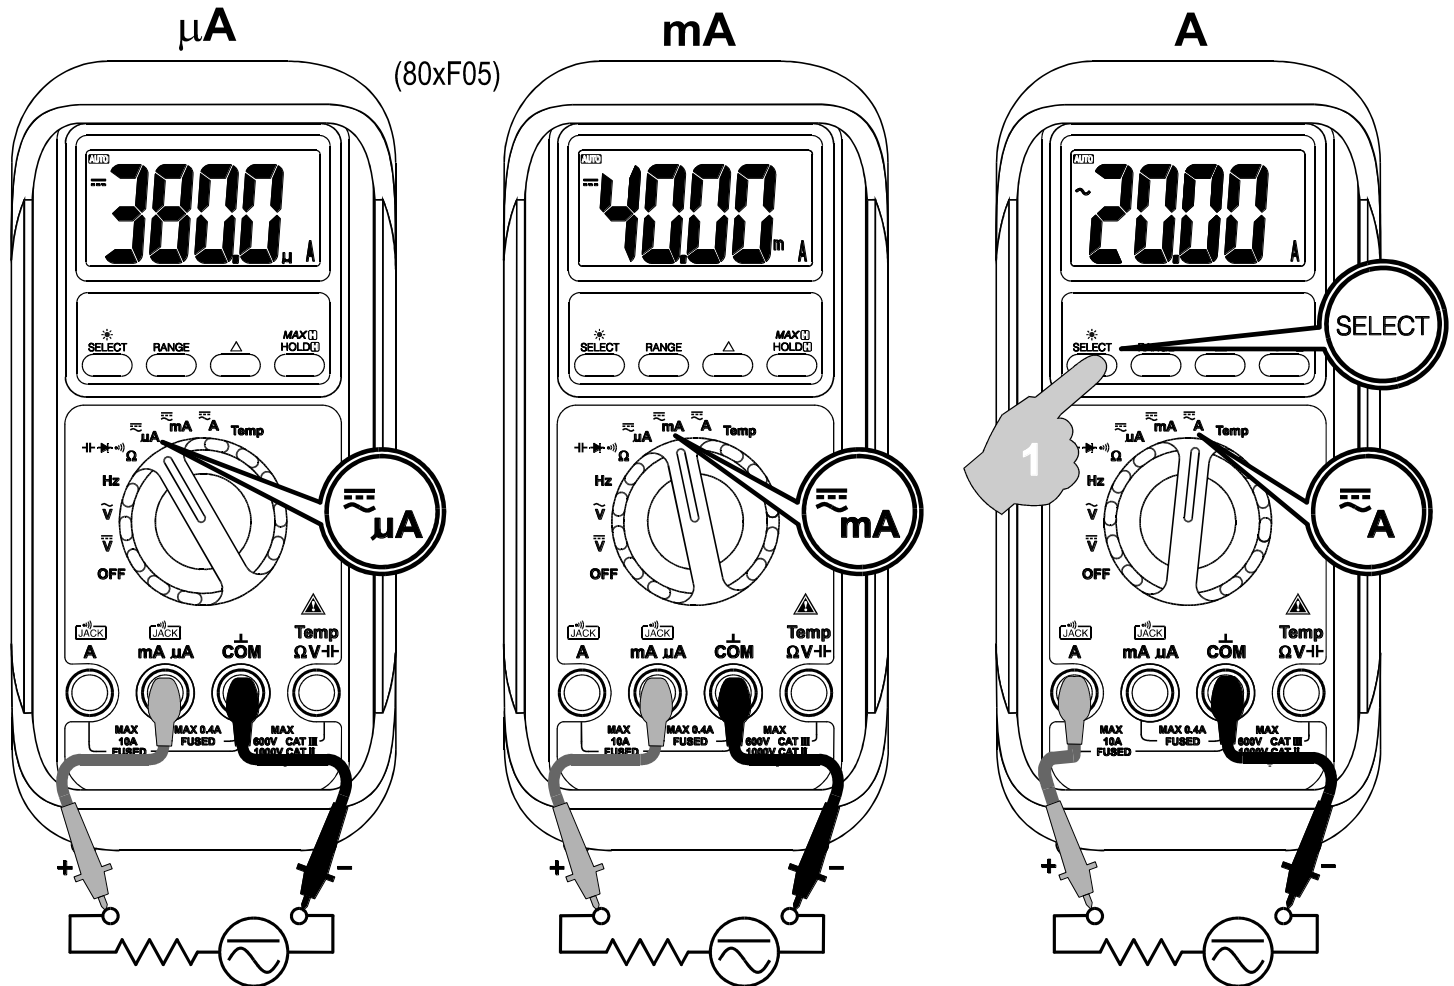

CAUTION


When measuring a 3-phase system, special attention should be taken to the phase-to-phase voltage which is significantly higher than the phase-to-earth voltage. To avoid exceeding the voltage rating of the protection fuse(s) accidentally, always consider the phase-to-phase voltage as the working voltage for the protection fuse(s).

Beep-Jack™ Input Warning

The meter beeps to warn the user against possible damage to the meter due to improper connections to the μA , mA, or A input jacks when other function (like voltage function) is selected.

Temperature function (Models 806s & 807s only)

Be sure to insert the banana plug type-K temperature bead probe Bkp60 (Optional purchase) with correct $+$ $-$ polarities. Defaults at degree C (Celsius). Press SELECT button momentarily to select degree F (Fahrenheit). You can also use a plug adapter Bkb32 (Optional purchase) with banana pins to type-K socket to adapt other type-K standard mini plug temperature probes.

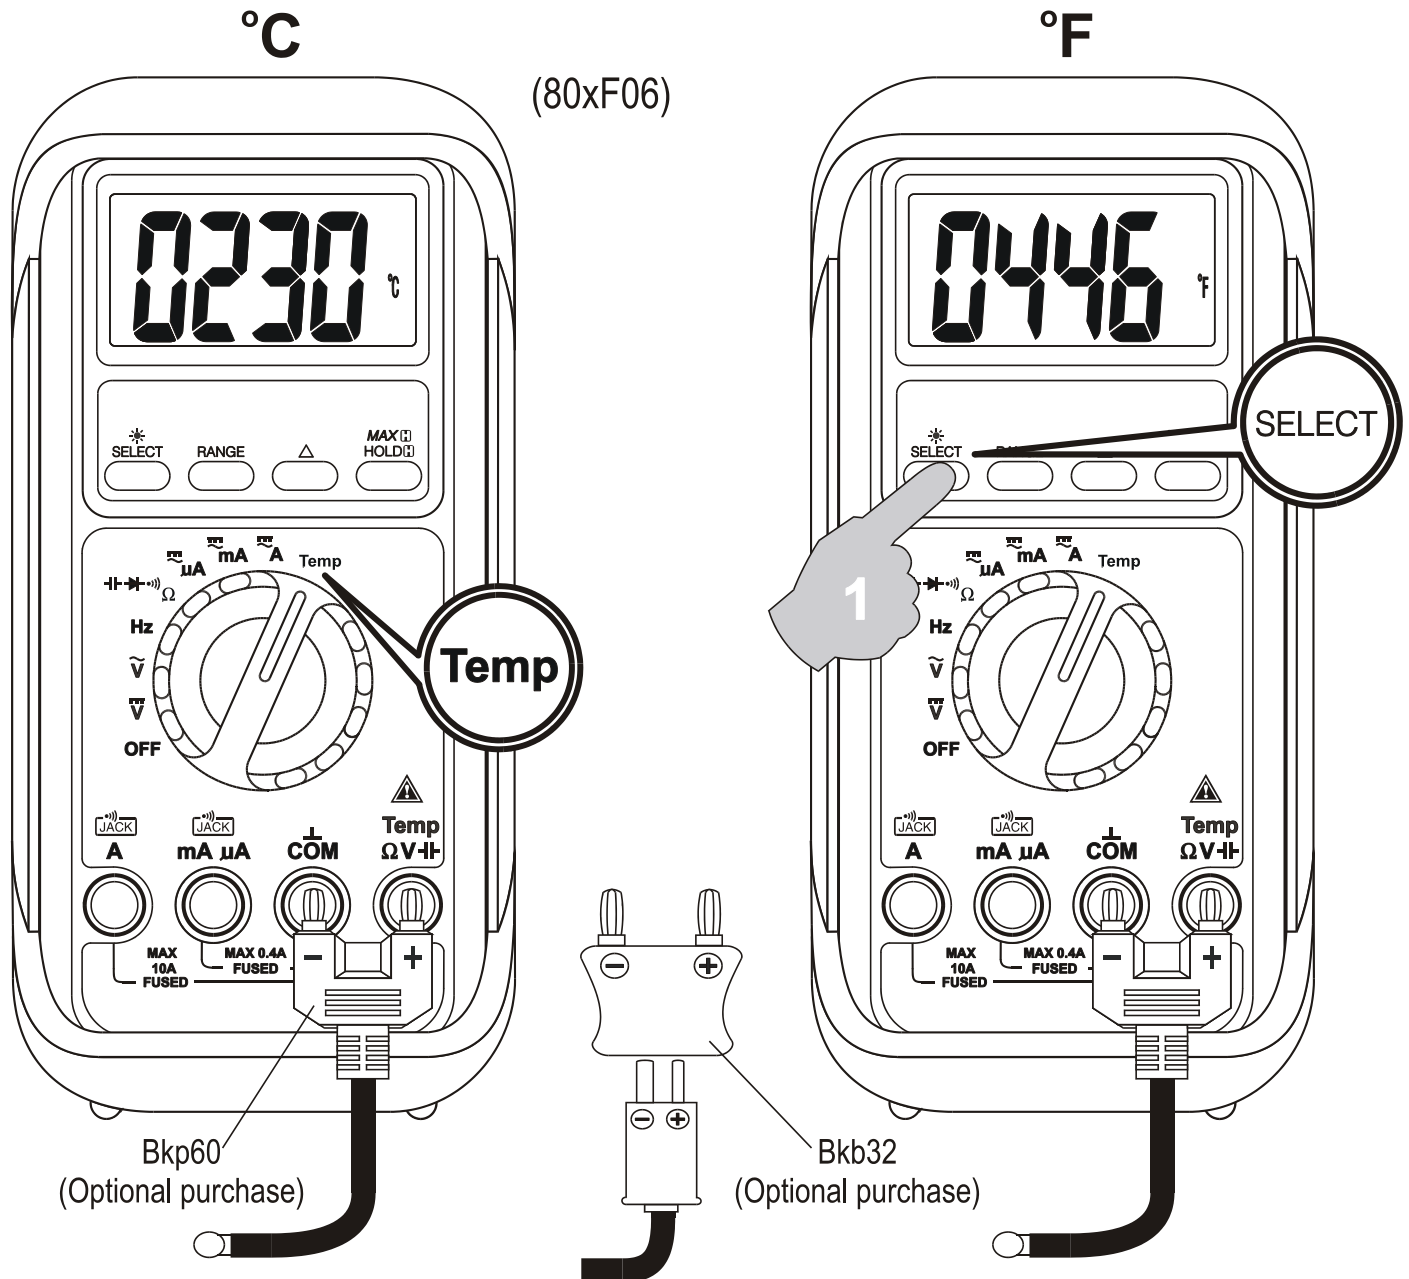

Relative zero Δ mode

Relative zero Δ mode allows the user to offset the meter consecutive measurements with the displaying reading as the reference value. The display will now show readings relative to the stored reference value. That is, display = reading - stored value. Press the Δ button momentarily to activate or to exit relative zero mode.

Backlight display (Model 807s only)

Press the **SELECT** button for 1 second or more to turn on or off the display backlight function.

Manual or Auto-ranging


Press the **RANGE** button momentarily to select manual-ranging mode, and the meter will remain in the range it was in, the LCD annunciator **AUTO** turns off. Press the button momentarily again to step through the ranges. Press and hold the button for 1 second or more to resume auto-ranging mode.

Note: Manual ranging mode feature is not available in Hz & Cx functions.

HOLD

The hold feature freezes the display for later view. Press the **HOLD ** button momentarily to activate or to exit the hold feature.

MAX

The max feature compares and displays the measured maximum value as fast as 25ms in a single range, and with automatic up range capability. Press the **MAX ** button for 1 second or more to activate or to exit the max feature in the voltage or current functions.

Sleep Mode

The meter will enter a low power consumption sleep mode automatically to extend battery life after approximately 30 minutes of no rotary-switch or push button operations. To wake up the meter from sleep mode, press any buttons momentarily or turn the rotary-switch to an adjacent position. Always set the rotary-switch to the OFF position manually when the meter is not in use.

5) MAINTENANCE

WARNING

To avoid electrical shock, disconnect the meter from any circuit, remove the test leads from the input jacks and turn OFF the meter before opening the case. Do not operate with open case.

Cleaning and Storage

Periodically wipe the case with a damp cloth and mild detergent; do not use abrasives or solvents. If the meter is not to be used for periods of longer than 60 days, remove the batteries and store them separately

Trouble Shooting

If the instrument fails to operate, check batteries and test leads etc., and replace as necessary. Double check operating procedure as described in this user's manual.

If the instrument voltage-resistance input terminal has subjected to high voltage transient (caused by lightning or switching surge to the system) by accident or abnormal conditions of operation, the series fusible resistors will be blown off (become high impedance) like fuses to protect the user and the instrument. Most measuring functions through this terminal will then be open circuit. The series fusible resistors and the spark gaps should then be replaced by qualified technician. Refer to the LIMITED WARRANTY section for obtaining warranty or repairing service.

Battery and Fuse replacement

Battery use:

Standard 1.5V AAA Size (NEDA 24A or IEC LR03) battery X 2


Fuse use:

Fuse (FS1) for μ mA current input:

0.4A/1000V ac & dc, IR 30kA, F fuse, or better; Dimension: 6 x 32 mm

Fuse (FS2) for A current input:

11A/1000V ac & dc, IR 20kA, F fuse, or better; Dimension: 10 x 38 mm

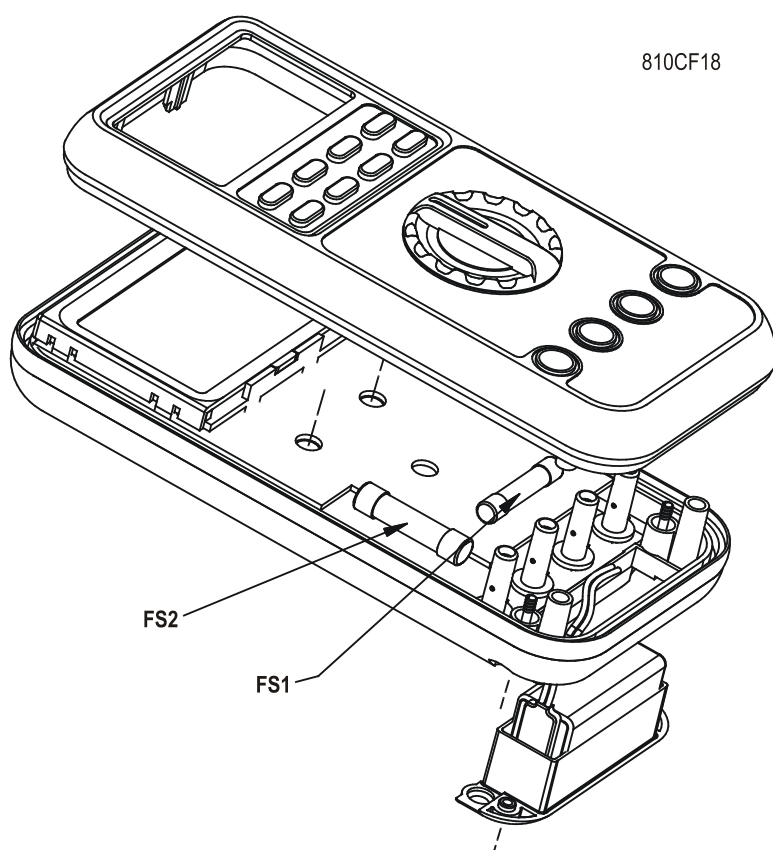

Battery replacement for models with battery access door:

Loosen the 2 screws from the battery access door of the case bottom. Lift the battery access door and thus the battery compartment up. Replace the battery. Re-fasten the screws.

Fuse replacement (and also Battery replacement for splash proof version without battery access door):

Loosen the 4 screws from the case bottom. Lift the end of the case bottom nearest the input jacks until it unsnaps from the case top. Replace the blown fuse(s) and/or the battery.

Replace the case bottom, and ensure that all the gaskets are properly seated and the two snaps on the case top (near the LCD side) are engaged. Re-fasten the screws.

6) Specifications

General Specifications

Display : 3-3/4 digits 4000 counts LCD display

Polarity : Automatic

Update Rate : 3 per second nominal

Operating Temperature : 0°C to 40°C

Relative Humidity : Maximum relative humidity 80% for temperature up to 31°C decreasing linearly to 50% relative humidity at 40°C

Altitude : Operating below 2000m

Pollution degree : 2

Storage Temperature : -20°C to 60°C, < 80% R.H. (with battery removed)

Temperature Coefficient : nominal 0.15 x (specified accuracy)/ °C @ (0°C -18°C or 28°C -40°C), or otherwise specified

Sensing : Average sensing for **Models 805s & 806s**. True RMS for **Model 807s**

Safety : The meter protection rating, against the users, is double insulation per **IEC/UL/EN61010-1 Ed. 3.0, IEC/EN61010-2-030 Ed. 1.0, IEC/EN61010-2-033 Ed. 1.0, IEC/UL/EN61010-031 Ed. 1.1 and CAN/CSA-C22.2 No. 61010-1-12 Ed. 3.0** to Category II 1000 Volts, CAT III 600Volts and CAT IV 300Volts AC & DC.

Terminals (to COM) measurement category:

V / A / mA μ A : Category II 1000V, CAT III 600V and CAT IV 300V AC & DC.

Overload Protections :

μ A & mA : 0.4A/1000V DC/AC rms, IR 30kA @ 1000V DC/AC rms

A : 11A/1000V DC/AC rms, IR 20kA @ 1000V DC/AC rms

V : 1100V DC/AC rms

Hz, Ohm & others : 1000V DC/AC rms

Transient protection : 6kV (1.2/50 μ s surge)

Power Supply : 1.5V AAA Size (NEDA 24A or IEC LR03) battery X 2

Power Consumption : 3.2 mA typical

Low Battery : Below approx. 2.4V

E.M.C. : Meets EN61326(1997, 1998/A1), EN61000-4-2(1995), and EN61000-4-3(1996)

In an RF field of 3V/m:

Capacitance function is not specified

AC 4.000V range: Total Accuracy = Specified Accuracy + 700 digits

AC 400.0 μ A range: Total Accuracy = Specified Accuracy + 300 digits

Other function ranges: Total Accuracy = Specified Accuracy + 40 digits

Performance above 3V/m is not specified

Sleep Mode Timing : Idle for 30 minutes

Sleep Mode Consumption : 300 μ A typical for **Models 805s & 806s**; 360 μ A typical for **Model 807s**

Dimension : L186mm X W87mm X H35.5mm; L198mm X W97mm X H55mm with holster

Weight : 296 gm; 396 gm with holster

Special Features : 25ms Max Hold; Data Hold; Relative zero mode; Beep-jack™ input warning; Back-lighted display (**Model 807s** only)

Accessories : Test leads (pair), batteries installed, user's manual

Optional Accessories : Banana plug type-K bead probe Bkp60 x 1 (**Models 806s & 807s** only), Banana pins to type-K socket plug adapter Bkb32 (**Models 806s & 807s** only)

Electrical Specifications

Accuracy is \pm (% reading digits + number of digits) or otherwise specified, at 23°C \pm 5°C & less than 75% R.H.

¹⁾**Model 807s** True RMS accuracy of ACV & ACA is specified from 5 % (10% for AC400.0mV range) to 100 % of range, or otherwise specified. Maximum Crest Factor < 1.75 : 1 at full scale & < 3.5 : 1 at half scale, and with frequency components within the specified frequency bandwidth for non-sinusoidal waveforms

DC Voltage

RANGE	Accuracy
400.0 mV	0.3% + 4d
4.000V, 40.00V, 400.0V	0.5% + 3d
1000V	1.0% + 4d

NMRR : >50dB @ 50/60Hz

CMRR : >120dB @ DC, 50/60Hz,
Rs=1kΩ

Input Impedance : 10MΩ, 30pF nominal
(1000MΩ for 400.0mV range)

AC Voltage

RANGE	Accuracy ¹⁾
50Hz -- 500Hz	
400.0mV*	4.0% + 5d
4.000V, 40.00V, 400.0V	1.5% + 5d
1000V	4.0% + 5d

CMRR: >60dB @ DC to 60Hz, Rs=1kΩ

Input Impedance: 10MΩ, 30pF nominal

*Selection by RANGE button manually,
and is specified from AC 10mV (AC
40mV for True RMS **Model 807s**) and
up

Max Hold (Voltage & Current)

Specified accuracy ± 50 digits for
changes > 25ms in duration

DC Current

RANGE	Accuracy	Burden Voltage
400.0μA	2.0% + 5d	0.15mV/μA
4000μA	1.2% + 3d	0.15mV/μA
40.00mA	2.0% + 5d	3.3mV/mA
400.0mA	1.2% + 3d	3.3mV/mA
4.000A	2.0% + 5d	0.03V/A
10.00A*	1.2% + 3d	0.03V/A

*10A continuous, 20A for 30 second
max with 5 minutes cool down interval

AC Current

RANGE	Accuracy ¹⁾	Burden Voltage
50Hz -- 500Hz		
400.0μA	2.0% + 6d	0.15mV/μA
4000μA	1.5% + 4d	0.15mV/μA
40.00mA	2.0% + 6d	3.3mV/mA
400.0mA	1.7% + 4d	3.3mV/mA
4.000A	2.0% + 6d	0.03V/A
10.00A*	1.8% + 4d	0.03V/A

*10A continuous, 20A for 30 second
max with 5 minutes cool down interval

Diode Tester

Open Circuit Voltage	Test Current (Typical)
< 1.6 VDC	0.25mA

Type-K Temperature (Models 806s & 807s)

RANGE	Accuracy*
-20 °C TO 300 °C	2% + 3 °C
-4 °F TO 572 °F	2% + 6 °F

*Type-K thermocouple range & accuracy not included

Audible Continuity Tester

Audible threshold : between 10Ω and 120Ω

Ohms

RANGE	Accuracy
400.0Ω	0.8% + 6d
4.000kΩ, 40.00kΩ, 400.0kΩ	0.6% + 4d
4.000MΩ	1.0% + 4d
40.00MΩ	2.0% + 4d

Open Circuit Voltage : 0.4VDC typical

Capacitance

RANGE*	Accuracy**
500.0nF, 5.000μF, 50.00μF, 500.0μF, 3000μF	3.5%*** + 6d

*Additional 50.00nF range accuracy is not specified

**Accuracies with film capacitor or better

***Specified with battery voltage above 2.8V (approximately half full battery). Accuracy decreases gradually to 12% at low battery warning voltage of approximately 2.4V

Hz Frequency

RANGE*	Accuracy**
50.00Hz, 500.0Hz, 5.000kHz, 50.00kHz, 500.0kHz, 1.000MHz	0.5%+4d

*Additional 5.000Hz range accuracy & sensitivity are not specified

**Accuracy is specified at < 20VAC rms

Input Signal : Square wave with duty cycle > 40% & < 70%; or Sine wave Vrms AC

Sensitivity :

10Hz--20Hz : > Sine 0.9Vrms;

20Hz--500kHz : > 2.6Vp; or Sine 1.9Vrms;

500kHz--1MHz : > 4.2Vp; or Sine 3Vrms

Update Rate : 2 per second nominal

LIMITED WARRANTY

BRYMEN warrants to the original product purchaser that each product it manufactures will be free from defects in material and workmanship under normal use and service within a period of one year from the date of purchase. BRYMEN's warranty does not apply to accessories, fuses, fusible resistors, spark gaps, batteries or any product which, in BRYMEN's opinion, has been misused, altered, neglected, or damaged by accident or abnormal conditions of operation or handling.

To obtain warranty service, contact your nearest BRYMEN authorized agent or send the product, with proof of purchase and description of the difficulty, postage and insurance prepaid, to BRYMEN TECHNOLOGY CORPORATION. BRYMEN assumes no risk for damage in transit. BRYMEN will, at its option, repair or replace the defective product free of charge. However, if BRYMEN determines that the failure was caused by misused, altered, neglected, or damaged by accident or abnormal conditions of operation or handling, you will be billed for the repair.

THIS WARRANTY IS EXCLUSIVE AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESSED OR IMPLIED, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTY OR MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE OR USE. BRYMEN WILL NOT BE LIABLE FOR ANY SPECIAL, INDIRECT, INCIDENTAL OR CONSEQUENTIAL DAMAGES.



北京海洋兴业科技股份有限公司 (证券代码: 839145)

北京市西三旗东黄平路19号龙旗广场4号楼 (E座) 906室

电话: 010-62176775 62178811 62176785 邮编: 100096

传真: 010-62176619

邮箱: market@oitek.com.cn

企业官网: www.hxyyq.com

购线网: www.gooxian.com



公司官网



微信公众号



微信视频号